
Labeling on the device

Product:

MedDream

Product version: **8.4.0**

Document version: **1.0**

Date: **2024-04-24**

Author: **PM Raimundas Mikalauskas**

Checked/ controlled/ evaluated by:

| Name | Date | Signature |
|--------------------|------------|-----------|
| QM Laura Baronienė | 2024-04-24 | |

Approved by:

| Name | Date | Signature |
|--------------|------|-----------|
| Not required | | |

Labeling on the device

Medical software MedDream does not have a tangible form. The only way to show information about manufacturer is to place this information in the „User Manual“ (as shown in Figure 1 “Information window” tab “ABOUT” and tab “REP”: annex No 1 to this document) and to make it visible by the software usage.

Information window tab “ABOUT” will display information mentioned below:

1. Full product name;
2. Version;
3. Release date;
4. UDI;
5. Medical device class;
6. ID of the notified body;
7. License to;
8. Concurrent connections;
9. Functions;
10. Valid to – empty if there is no termination in time;
11. Update to – date till the technical support and updates are provided;
12. Manufactured by – Softneta UAB contacts.
13. Distributed by – Distributor contacts, if applicable (and distributor brand name, if applicable).

Information window tab “REP” is intended to display about authorized representative in different countries.

Annex No 1 to Labeling on the device: Information window tab „ABOUT“ and tab „REP“

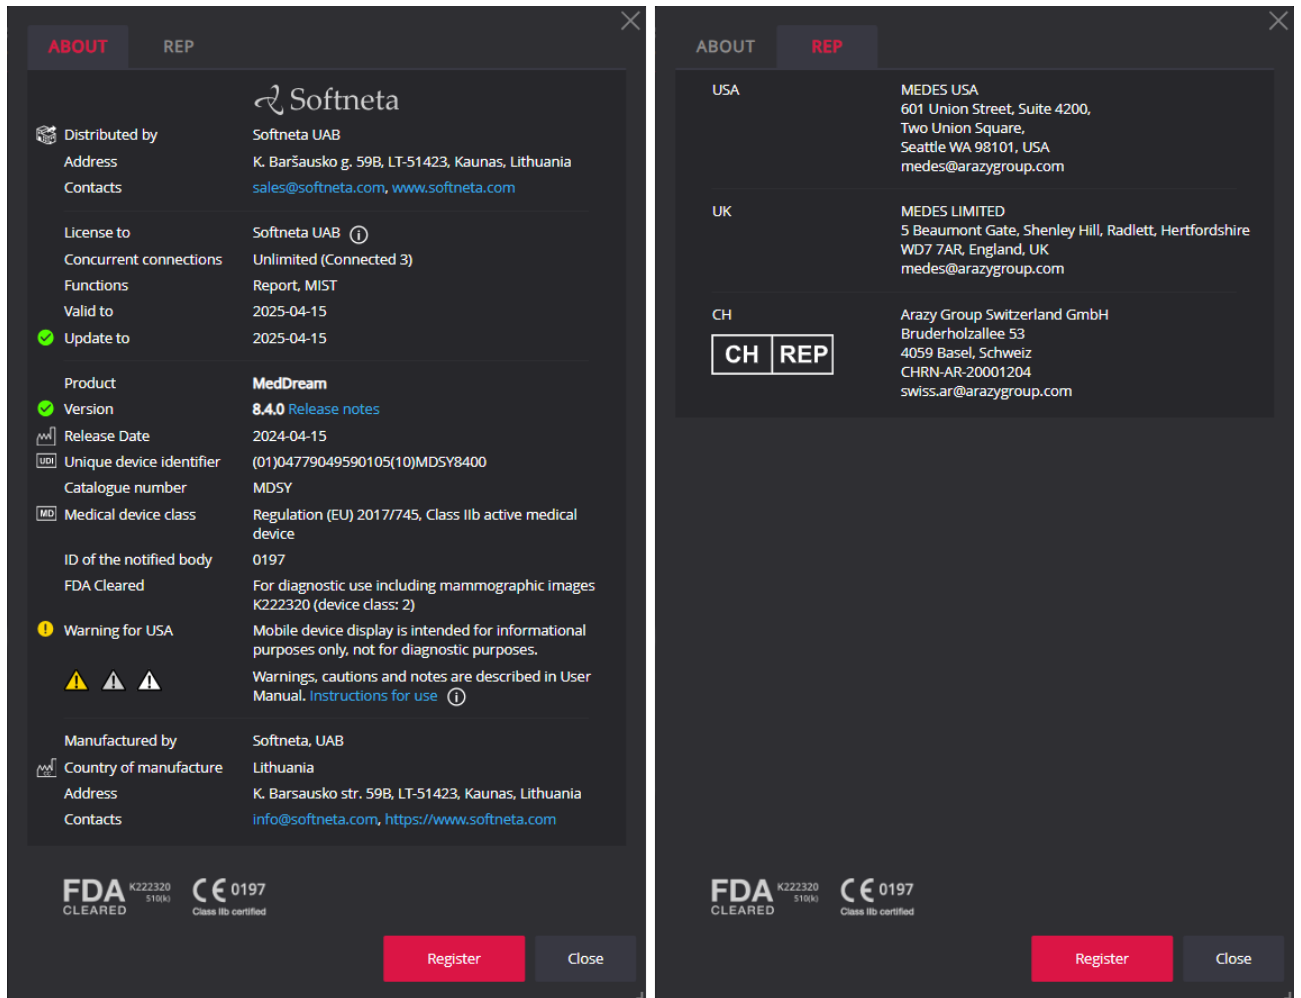


Figure 1. Information window tab “ABOUT” and tab “REP”